



Content

About us 04

Ultrasonic Bone Surgery 08



About us

"Today we are innovating because tomorrow we could be the patient": it is in this spirit that the ACTEON® medical team works constantly to develop its products.

Technology should have only one purpose: to help us live better. This is why we base our approach on the greatest respect of patients and their safety.

"Inspired by the practitioners, dedicated to their patients."



our vision our mission

We believe healthcare is first and foremost about quality of life. Medical treatments are more than just procedures, they restore health, comfort, confidence and happiness and improves life of millions of patients every year. Our vision is to pave the way of a more human-centered healthcare industry based on proactive lifetime care.

To remain at the top of their game and focus on what matters most, healthcare professionals trust integrated solutions that empower them and improve their practices on a daily basis. We provide comprehensive, intuitive workflow solutions that put technology at the service of people and help healthcare professionals restore patients'health effectively, efficiently, and economically.



Ultrasonic Bone Surgery

Piezotome® solo m+	10
Device	10
Footswitch & Handpiece	11
Clinical kits	12
Rhinoplasty tips «Essential»	14
Rhinoplasty tips «Expert»	15
Rhinoplasty tips «Preservation»	16
CMF tips «Essential»	17
All tips	18
Osteotomy tips	18
Osteoplasty tips	20
Bone remodeling / Drilling tips	21
Membrane detachment tips	22
Tip measuring guide	23
Additional products	24

Ultrasonic Bone Surgery 10 Ultrasonic Bone Surgery

Piezotome® solo m+

Device



Reference	Description
F57850	Piezotome® Solo M+ CEE
F57853	Piezotome® Solo M+ AUS
F57856	Piezotome® Solo M+ US
F57859	Piezotome® Solo M+ UK

- Medical device of class IIb CE 0459 according to Medical Device Directive 93/42/EEC
- Manufacturer: SATELEC, a company of ACTEON® Group

SPECIFICATION OF THE DEVICE

F57850 / F57853 / F57856 / F57859

- Dimensions (W x H x D): 378 x 136 x 306mm
 With brackets: 378 x 460 x 306mm
- Weight: 3700 g
- Screen dimensions (W x H): 115 x 86 mm
- LCD black & white screen
- 4 power modes
- 4 programmable buttons
- Irrigation flow rate: 0 to 120 ml/min
- Reset to manufacturer settings
- Supply voltage: 100 230 VAC

- Power supply frequency: 50 Hz / 60 Hz
- Power consumption: 150 VA to 230 VAC
- No-load voltage: 250 V
- Minimum output frequency: 28 kHz
- Amplitude: 20 to 200 µm
- Internal fuse not accessible to the user: 1 fuse F1:
 5mm x 20mm 10 AT / 250 VAC
- Fuse (mains connector): 2 fuses 5mm x 20mm 2 AT for 100 to 230 VA

Piezotome® solo m+

Handpiece & Footswitch



Reference	Description
F12860	Piezotome® M+ handpiece

11

- Medical device of class IIb CE 0459 according to Medical Device Directive 93/42/EEC
- Manufacturer: SATELEC, a company of ACTEON® Group

SPECIFICATION OF THE PIEZOTOME® M+ HANDPIECE

F12860

- Dimensions (L): 130 mm
- Weight: 100 g
- With cord: 265 g

- Cord length: 2900mm
- 6 ceramic rings
- Cold LED light (power): 100 000 LUX



Reference	Description
F57851	Piezotome® Solo M+ footswitch

SPECIFICATION OF PIEZOTOME® SOLO M+ FOOTSWITCH

F57851

- Cord length: 2900mm
- Dimensions (W x H x D): 173 x 140 x 176mm
- Weight: 1000 g
- Light: remains active approx. 9 secs after the footswitch is released
- Multifunction footswitch:
 - Power modes
 - ON/OFF ultrasound
- Protection rating: IPX6

The footswitch is delivered with its corresponding device Piezotome® is a registered trademark of SATELEC SATELEC® is a registered trademark of SATELEC

Ultrasonic Bone Surgery

Clinical kits Introduction

INTENDED USE

M+ tips can be used for osteotomy, osteoplasty, decortication, drilling, shaping and smoothing of teeth and bone in various surgical procedures, including but not limited to general, orthopaedic, otolaryngological, maxillofacial, oral, hand and foot, neurosurgery, spinal and plastic/reconstructive surgeries.

SPECIFICATION OF REUSABLE NON-STERILE TIPS

- Non-sterile tips can be used up to 5 times
- Refer to cleaning, disinfection and sterilization protocols for SATELEC® tips



REGULATORY & ENVIRONMENT

- Class IIb according to the European Directive 93/42/ EEC
- Designed and manufactured in accordance with an EN ISO 13485-certified quality assurance system
- Documentation complies with European regulation No.207/2012
- Manufacturer: SATELEC®, a company of ACTEON® Group (France)



14 Ultrasonic Bone Surgery Ultrasonic Bone Surgery

Clinical kits

Rhinoplasty tips «Essential»



Reference	Description
F87681	Rhinoplasty kit "Essential" non-sterile 6 tips - 5 times reusable

Metallic support included



Clinical kits

Rhinoplasty tips «Expert»



Reference	Description
F87689	Rhinoplasty kit "Expert" non-sterile 9 tips - 5 times reusable

Metallic support included

15









	RHS1	RHS2Hb	RHS2Fb	RHS3L	RHS3R
Reference	F87688	F87686	F87687	F87677	F87678
Length (mm)	28	33.7	33.7	30	30
Offset (mm)	12.2	11	11	10	10
Width (mm)	3.5	3.5	3.5	5	5
Thickness (mm)	0.55	1.3	0.9	0.6	0.6



F87683

31.5

9.5

2.6

0.5

Reference Length (mm)

Offset (mm)

Width (mm)

Thickness (mm)



RHS4R

F87682

31.5

9.5

2.6

0.5



0.5


TH-RH-95	RHS6	
RHS5	RHS6	
F87679	F87680	
34	27	
11	17	
26	•	

0.5

Ultrasonic Bone Surgery 16 Ultrasonic Bone Surgery 17

Clinical kits

Rhinoplasty tips «Preservation»

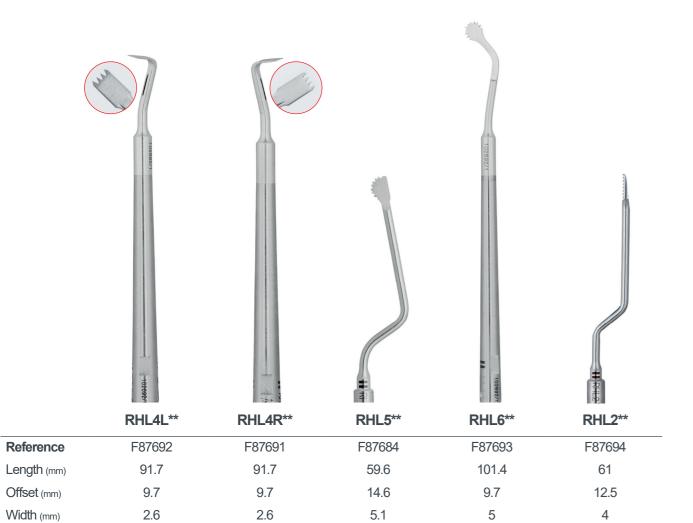

0.6

0.6

1.1

Clinical kits

CMF tips «Essential»



Reference	Description
F57803	CMF kit non-sterile
F37603	6 tips - 5 times reusable

Metallic support included



0.4

Thickness (mm)


^{**}Please contact us to find out the availability of the product in your country

Ultrasonic Bone Surgery 18 Ultrasonic Bone Surgery 19

All tipsOsteotomy tips





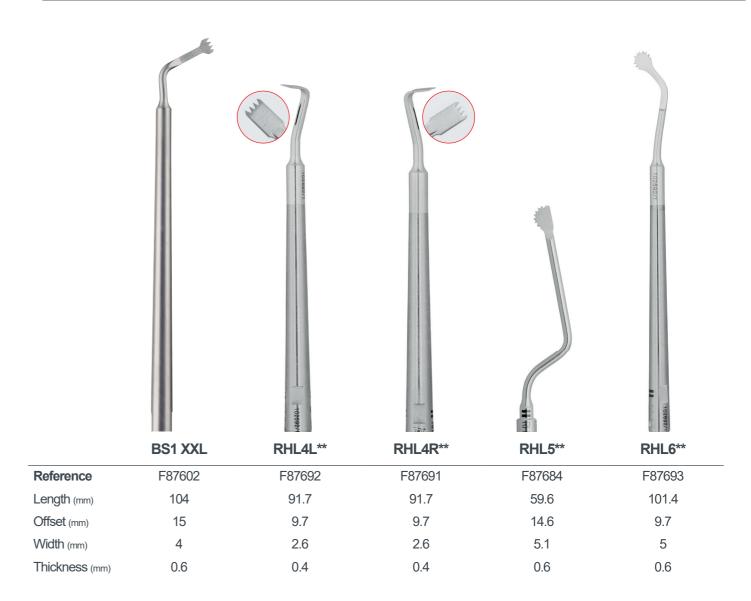




^{**}Please contact us to find out the availability of the product in your country

Ultrasonic Bone Surgery 20 Ultrasonic Bone Surgery 21

All tipsOsteoplasty tips

BS4 BS6 RHS1 RHS2Hb RHS2Fb F87615 F87617 F87687 Reference F87688 F87686 28 28 33.7 Length (mm) 31 33.7 Offset (mm) 12.6 11.9 12.2 11 11 Width (mm) 4 3.5 3.5 3.5 3.5 Thickness (mm) 0.7 0.55 0.55 1.3 0.9

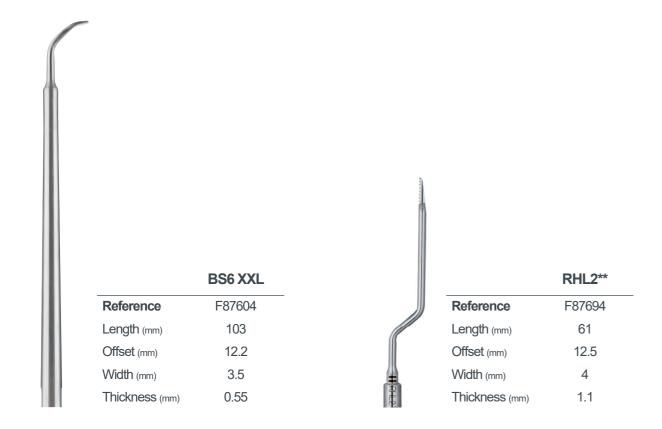

All tips

Bone remodeling / Drilling tips

	H OE3	081	DB 2	III THOS	11 812
	CE3	DB1	DB2	RHS6	SL2
Reference	F87653	F87610	F87609	F87680	F87619
Length (mm)	29.8	27	30.7	27	28
Offset (mm)	10.2	17	20.1	17	14
Width (mm)	•	•	•	•	•
Thickness (mm)	0.85	0.6	2.3	0.5	1.5

^{**}Please contact us to find out the availability of the product in your country

Ultrasonic Bone Surgery Ultrasonic Bone Surgery

All tips

Membrane detachment tips

	SL3	SL4	SL5
Reference	F87620	F87621	F87622
Length (mm)	31	29.1	30.9
Offset (mm)	12	10.2	11.1
Width (mm)	5	4	4
Thickness (mm)	0.4	0.65	0.65



Tip measuring guide

	Length (a)	Offset (b)	Width (c)	Thickness (d)
Osteotomy	a	b	C C C C C C C C C C C C C C C C C C C	d d
Osteoplasty	a	b	or C	or d
Bone remodeling / Drilling	a	b		d d
Membrane detachment	a	b	c	or

Ultrasonic Bone Surgery 24 Ultrasonic Bone Surgery 25

Additional products



Reference	Description
F57802	Autoclavable metallic cassette, Piezotome® M+ LED handpiece, 3m cord, M+ wrench

- Medical device of class IIb CE 0459 according to Medical Device Directive 93/42/EEC
- Manufacturer: SATELEC, a company of ACTEON[®] Group



Reference	Description
E27157	Autoclavable M+ metallic empty cassette

Not a Medical Device



Reference	Description
F59926	Set of 1 disposable sterile line
	With clips and perforators
F59925	Set of 5 disposable sterile lines
	With clips and perforators

Accessories of Medical Device, Class Is as per Medical Device Directive 93/42/EEC

Additional products



Reference	Description
F88474	Tips metallic support M+ 10 slots Without tip and marking

Not a Medical Device



Reference	Description
F88445	Tips metallic support M+ 6 slots Without tip and marking

Not a Medical Device



Reference	Description
F00398	M+ Flat key

Not a Medical Device

Ultrasonic Bone Surgery 26 Ultrasonic Bone Surgery 27

Additional products



Reference	Description
E27113	Bracket M+
	Component of Class Ilb Medical Device as per Medical Device Directive 93/42/EEC



Reference	Description
F87903	M+ Protective sleeve For extra long tips (XXL)
Not for sale in the US	



Reference	Description
E00052	Rhinoplasty model - Density 1

Not a Medical Device

Additional products



Reference	Description
E12813	Nose cone for Piezotome® M+ handpiece

Spare parts of Medical Device



Reference	Description
E12812	Light guide for Piezotome® M+ handpiece

Spare parts of Medical Device



Reference	Description
F12821	LED Ring M+

Spare parts of Medical Device



SATELEC

A company of ACTEON® Group

17 Av. Gustave Eiffel, ZI Phare 33700 Mérignac France

acteonmed@acteongroup.com

Follow-us

